

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

JUL 09 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130584

Supervisor/Operator Performing the Verification Procedure:

Name Supt. James R. R. Rea

ID# 3161

Date 06-30-09

A Agency Kotzebue Police Department

Phone # 907-442-3352

Instrument Location Kotzebue Regional Jail 258d rm#107 Fourth Avenue Kotzebue, AK 99752

B

Alco S/N X172931

Target Value .084

High Pressure 0350

Alco Test Values:

.086
1st Alco

.086
2nd Alco

Signature _____

Supt. James R. R. Rea
(OVER)

003
7/14/09

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of Jul, 2009.

Carolyn M. Noland (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska



Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130584

(CONTINUED FROM FRONT PAGE)


C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

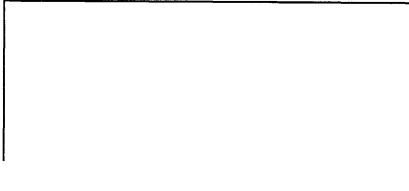

Breath Test Record			
Serial Number	130584	Model	DataMaster
Location	OTZ1	Kotzebue Police Dept.	
Subject Information			
Last Name	Verification Of Cal	O.L. #	06302009
First Name	Verification Of Cal		
Operator Information			
Operator Name	Rea/James/Rt	Case	06302009
Operator #	3161	Department	OTZ1
Test Results			
Alco Target	084	Alco Serial	X172931
Nominal	0.085	Barometer	30.53
Dry Gas 1	0.086	Time:	18:06:53
Subject Alcohol	0.000	Time:	18:08:04
Dry Gas 2	0.086	Time:	18:09:10
		Test Type	V
		Test Date	06/30/2009
		Test Time	18:05:12
		Report	Y

DIAGNOSTIC CHECK



Diagnostic Test Record	
Serial Number	130584
Model	DataMaster
Location	OTZ1
Kotzebue Police Dept.	
Diagnostic Test Results	
Test Date	06/30/2009
Test Time	17:42:01
Computer	Okay
Program	Okay
Software Date	02/20/2001
Sample Chamber (C)	50
Breath Tube (C)	42
Barometer (in)	30.53
Flow Detector	Okay
High Speed Pump	Okay
Detector	Okay
Filter	Okay
Quartz	Okay
Calibration	Okay